

ATLANTIS™



Atlantis™ WebOrder

User guide

Contents

Atlantis™ WebOrder	
User registration	4
Entering an order	7
Order page 1 – Overview	8
Order page 2 – Items	10
Order page 3 – Parallelism	13
Order page 4 – Bill & ship	14
Order ticket	15
Hold for design approval	16
Later orders	17
Abutment screw	18
No rescan required	18
Rescan required	20
Account settings	22
Preferences	24
Design profiles	25
Add preferences	26
Enter new profile	27
Help	28
Emergence width options	29
Model type	29

This manual is designed as a guide for users of Atlantis™ WebOrder.

User registration

Welcome page

Enter www.atlantisweborder.com into your web browser.

Select language from the drop down menu.

For registered users, enter your account e-mail address and password and press **Go** button to log in.

New users must register to access Atlantis™ WebOrder.

Click the **Register** link to start the registration process.

ATLANTIS™
WebOrder

ASTRATECH
DENTAL
Get Inspired

Welcome to Atlantis™ WebOrder!

If you have an existing account, please enter your e-mail and password and press the "GO" button to begin. If you are not a registered user, click on the "Register" link to set up an account.

Login to enter an order

Email:

Password:

Remember me:

GO

[Register to use Atlantis™ WebOrder](#)

Choose your language:
English

Forgot your password?

For assistance, please contact Customer Service for [North America](#) or for [Canada/Asia/Australia](#).
[AstraTech Privacy Policy and Terms of Service](#)

Register page

You must register to gain access to the Atlantis™ WebOrder site by completing all required information on the **Register** page. This information may be edited at a later time by the account manager on the **My account** page.

Note: If **Bill to** or **Ship to** information is different than **Ordering address**, uncheck the box(es) to enter additional information. To complete your registration, the **Terms of Service** must be accepted by clicking the check box.

Register to Atlantis™ WebOrder

User

First name:

Last name:

Email:

Ordering Address

Business name:

Address 1:

Address 2 (optional):

Address 3 (optional):

City:

State/Province:

Postal code:

Country:

Phone:

Fax (optional):

Bill To

Same as order by:

Ship To

Same as order by: Same as bill to:

I accept the [Terms of Service](#)

REGISTER


Once you have completed entering in the required information, click on the **REGISTER** button. You will be redirected back to the **Welcome** page.

Confirmation

Upon completion of registration, the message below will appear.

Follow the instructions to verify your registration.

Upon verification, you will be directed to the Atlantis™ WebOrder **Welcome** page.

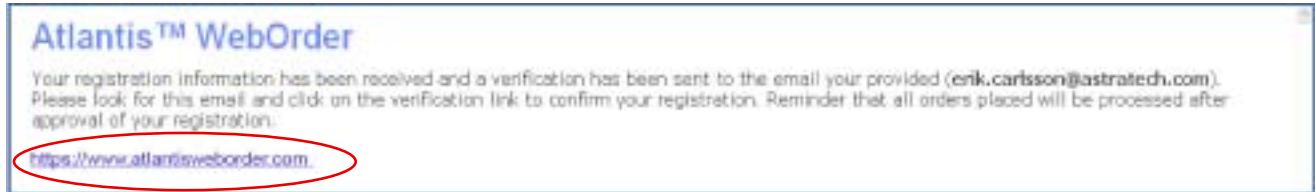


Orders

New orders are entered from the **Orders** page. Click the **Enter new order >>** link to begin.


You will be guided through the order process based on your specific selection.

- Click the **Save and exit** button at any time to save your entries and return later to complete and submit your order to Astra Tech
- Go directly to any order by clicking on the hyperlink in the **Patient or PO/Ref.** column
- Sort orders by clicking on the headers of any column
- If the status is SHIPPED under the **Status** column, clicking on the hyperlink will provide you with shipping details
- **Due date** indicates the day you should expect to receive the case

First time view.

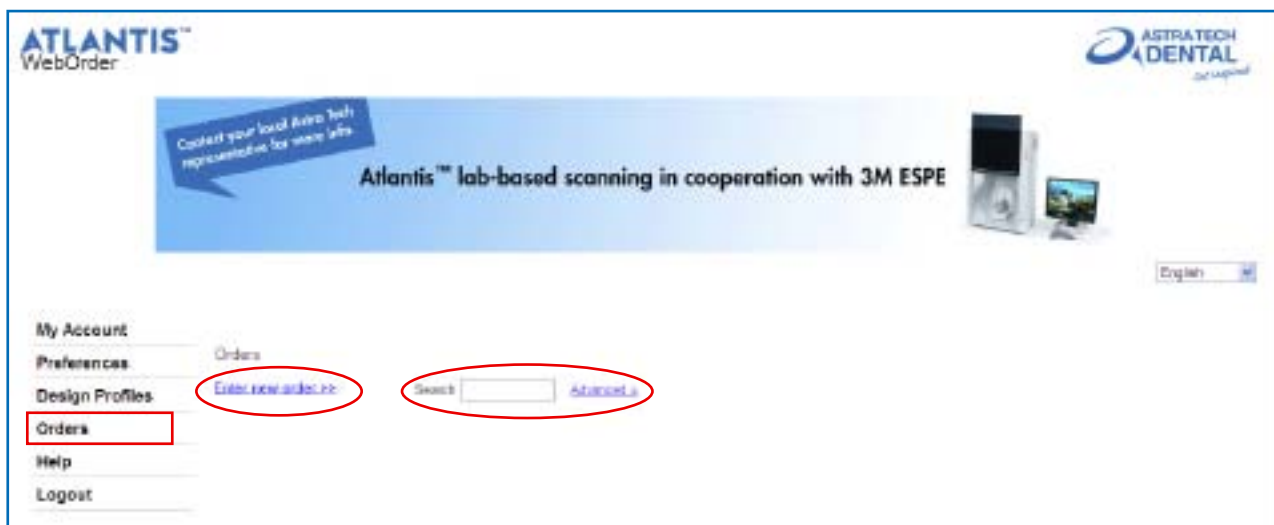

View showing list of entered cases.

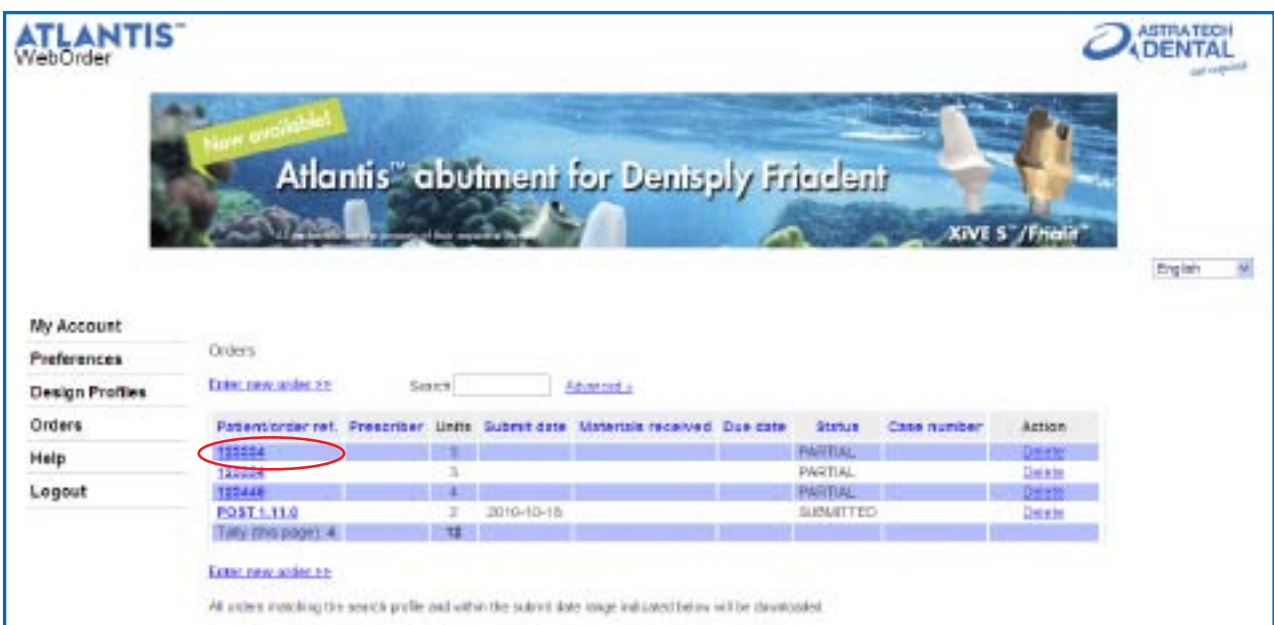

Entering an order

Order page 1 – Overview is used to enter initial case information.

Fields with an “*” and implant location(s) are required.

Process case – do not send images. Select this option for your case to be fully processed. Abutment design images will not be sent.

Hold case – send images. Select this option to receive images of your case for review and approval prior to fabrication.

Indicate the **Model Type** being sent by clicking the appropriate button.

Click the tooth number(s) to indicate where the implant(s) is located.

Note: The type of model you send for your Atlantis™ case will define the design options available to you.

If sending a stone model of soft tissue, only an emergence width option of No Tissue Displacement will be available.


If sending a stone model with no soft tissue captured, “Use Subgingival Depth” margin position will not be available. The only emergence width option will be Full Anatomical Dimensions.

Click **Next** to continue or **Save and Exit** to save your progress and return later to complete your order.

When **Hold case – send images** is selected, the **E-mail for abutment image notification** field is a mandatory field. This allows us to always have proper contact information should there be any questions or concerns during the abutment design process.

Account Users can also share case images in 2D or 3D. All e-mails for non-account users entered in the first field will receive access to 3D images for the case. All e-mails entered for non-account users in the second field will receive only 2D images.

Any requests or changes to abutment designs must be entered by an Account User within Atlantis™ WebOrder.

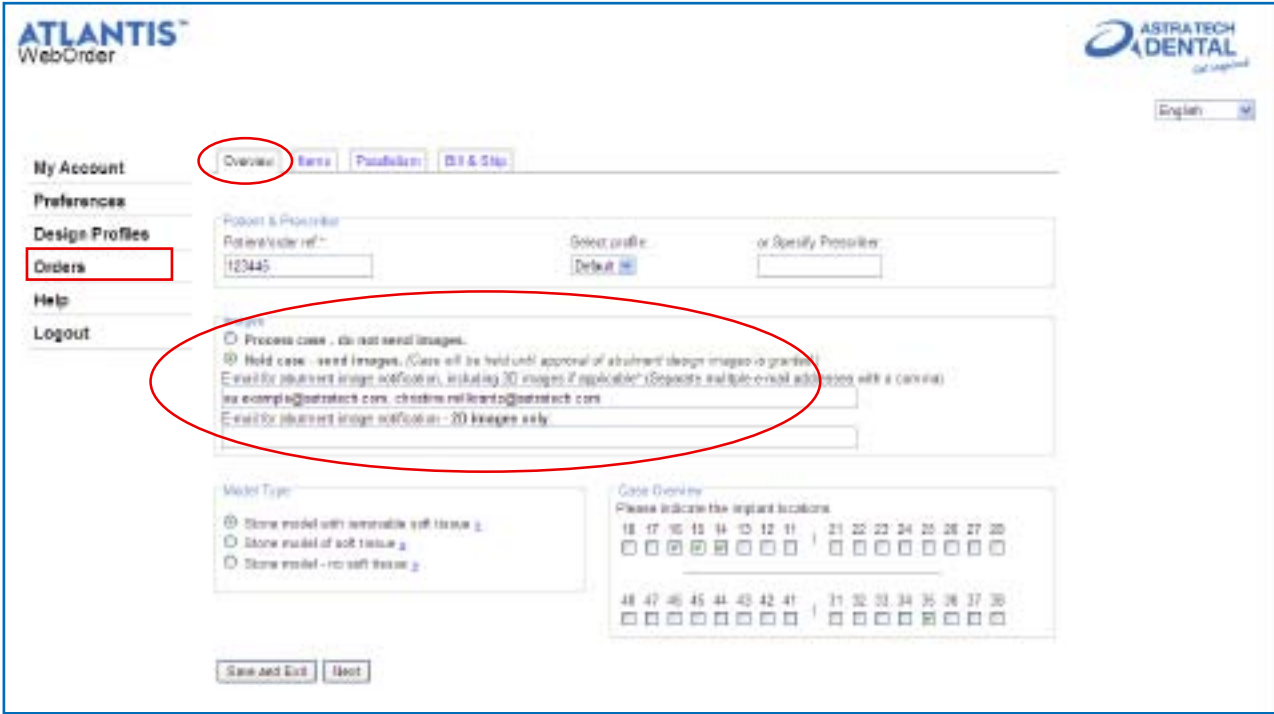


Entering an order

You can also choose to **Share case images** after a case has been submitted. To do so, click on the case from the Order List to open up the Orders/Show page. Click on the **Share case images...** link.




Once the **Share cases images...** link is clicked, the page will expand. Enter e-mail address. If you wish to send only 2D images, uncheck the **Share 3D?** box and click **Add email address and send image immediately >>** link.

In addition, any e-mail addresses (previously entered during the order entry process on the Overview page) will also be listed with a check box under this link for easy re-sending. If access was given in error during the order entry process, e-mails can be checked and deleted. This will deactivate the access link in the e-mail that was previously sent.

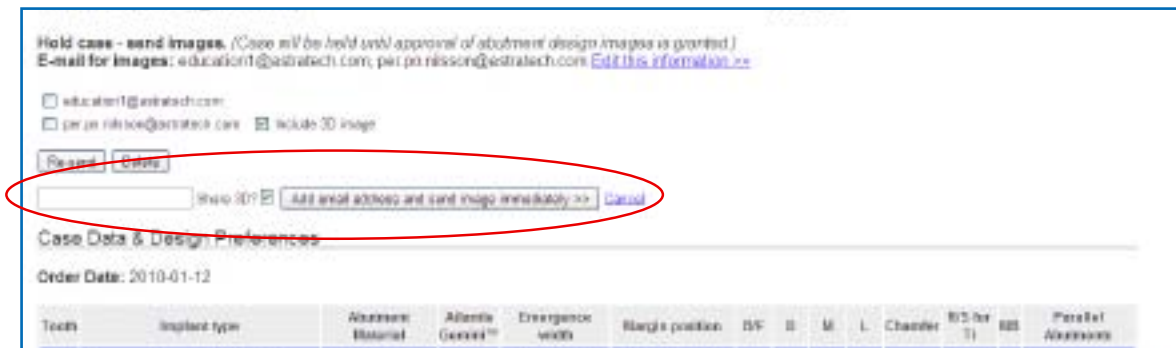

Order page 2 – Items is used to specify implant and abutment information per tooth.

Select **Implant type** and size for each tooth number from the implant selection table.

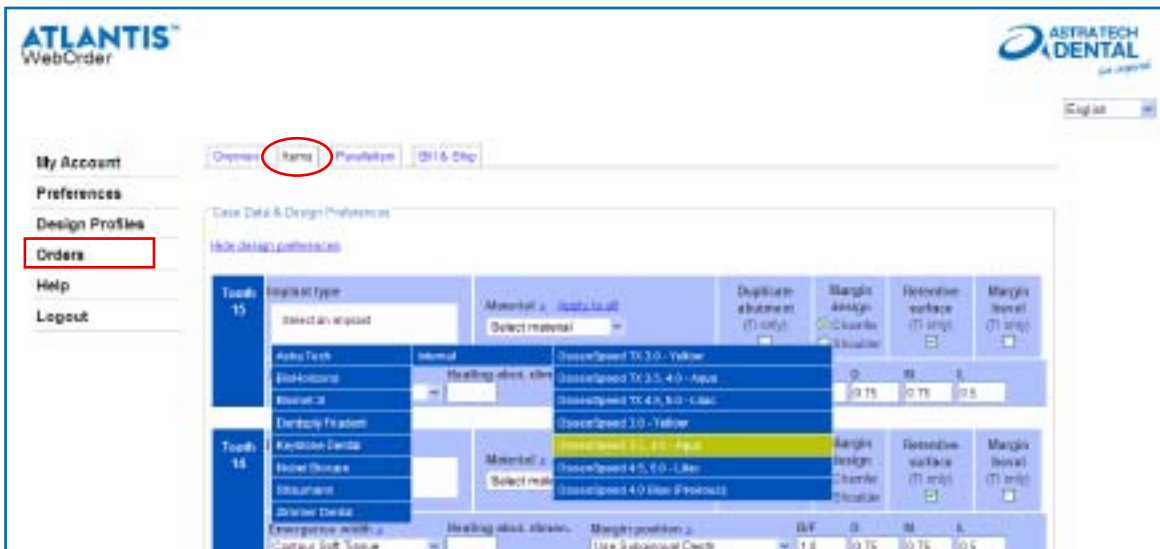

Then select either Cement-retained or Screw-retained under **Restoration type**.


Clicking on the >> brings up a pop-up image with additional information on the restoration options.

Select Material for each tooth number from the drop-down menu.


Note: Only corresponding materials available for the implant and restoration type selected will display.

Indicate if you want a duplicate of your Atlantis™ abutment by checking the **Duplicate abutment** box in addition to the material selection.

Changes made here will not alter your default preferences.

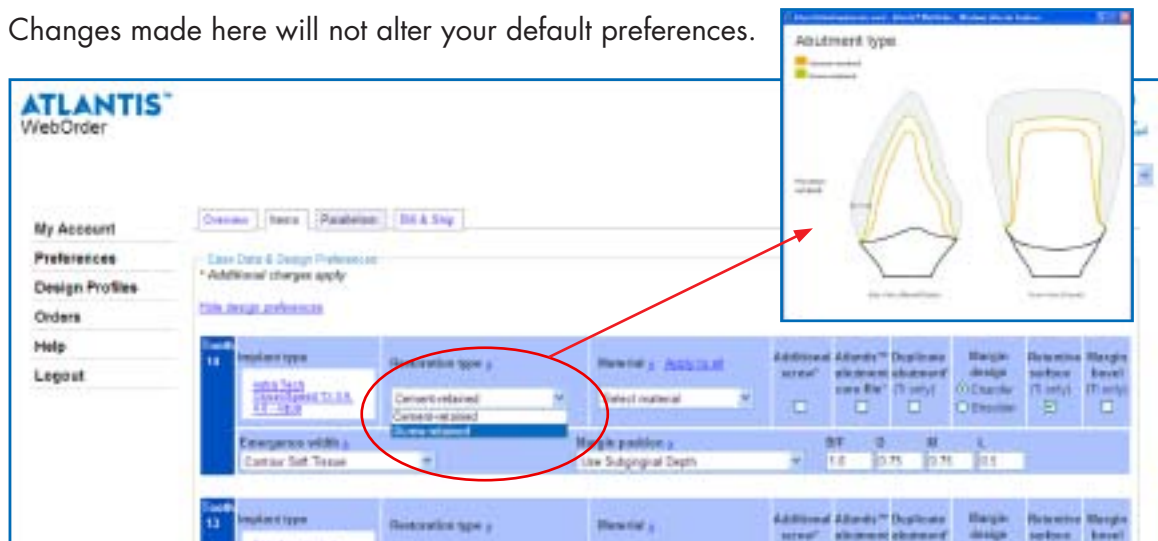

The Items page is defaulted to **Show design preferences**. If you do not want to see the details for each tooth, click the **Hide design preferences** link.

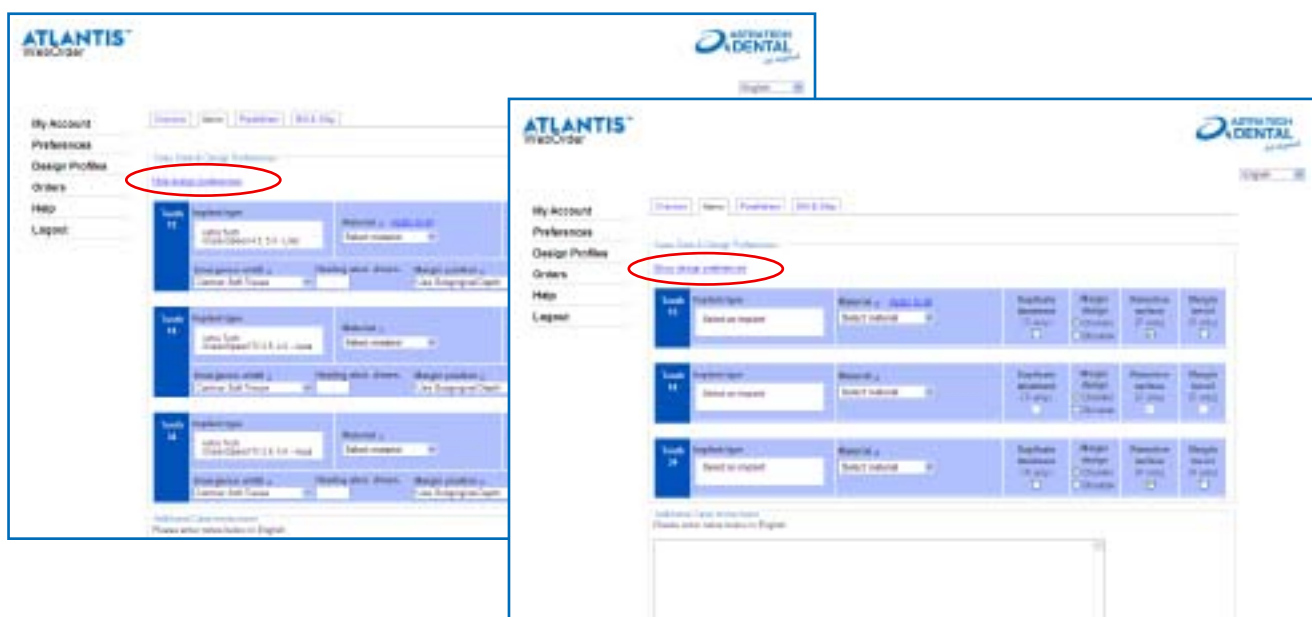


Click **Next** to continue or **Save and Exit** to save your progress and complete your order later.

Entering an order


Note: For zirconia abutments, a radius of 2.5 mm from the center of the implant to axial walls of existing dentition is required (0.5 mm total diameter).

Clicking on the >>> brings up a pop-up with additional information and/or illustration.


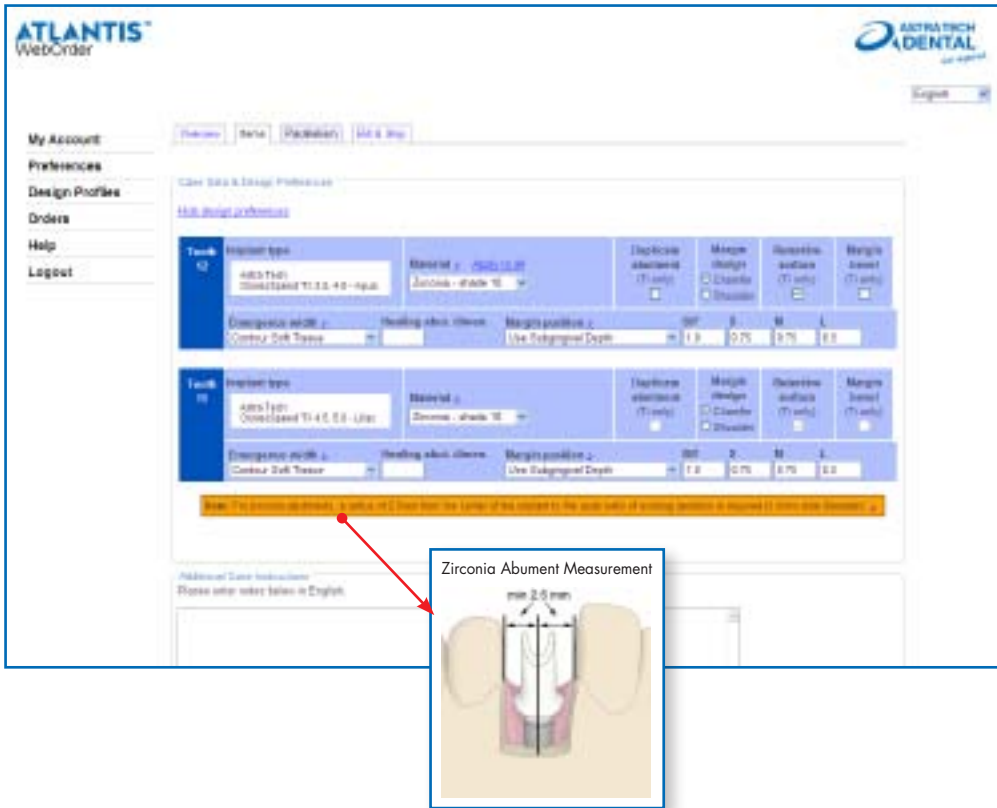


Select abutment material from the dropdown list.

Clicking on the >>> brings up additional information on the material options.

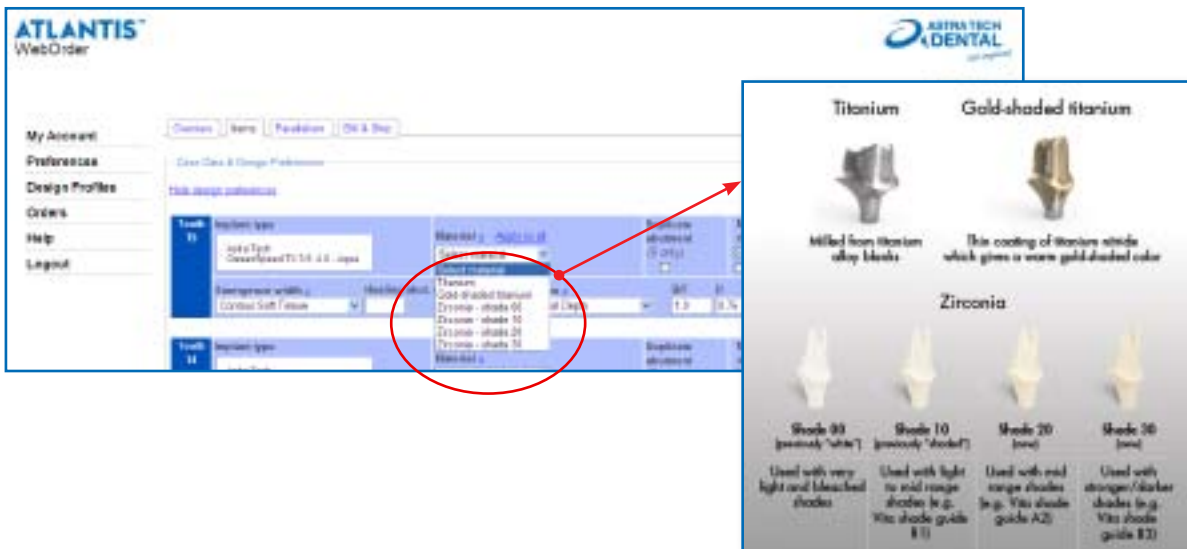

Order page 3 – Parallelism is used to indicate abutments that should be made parallel to each other by selecting them under the same “P” column. Parallel abutments are identified with the same color-coding on the tooth numbering chart for easy verification.

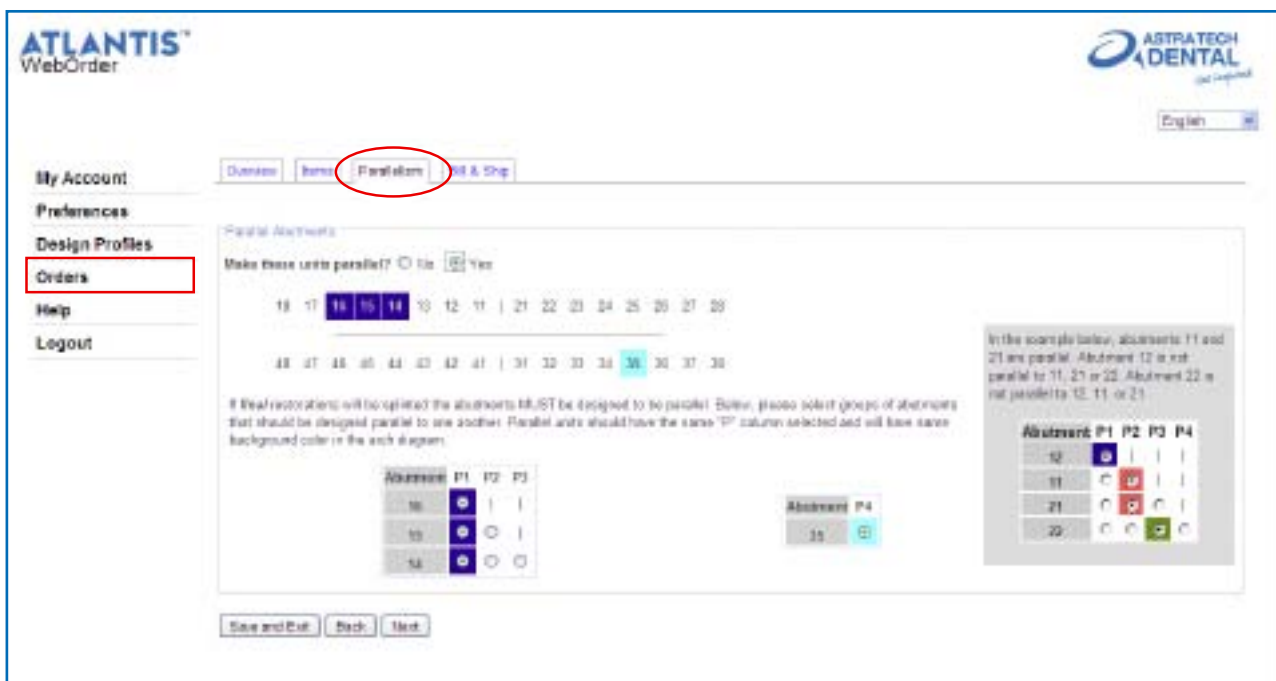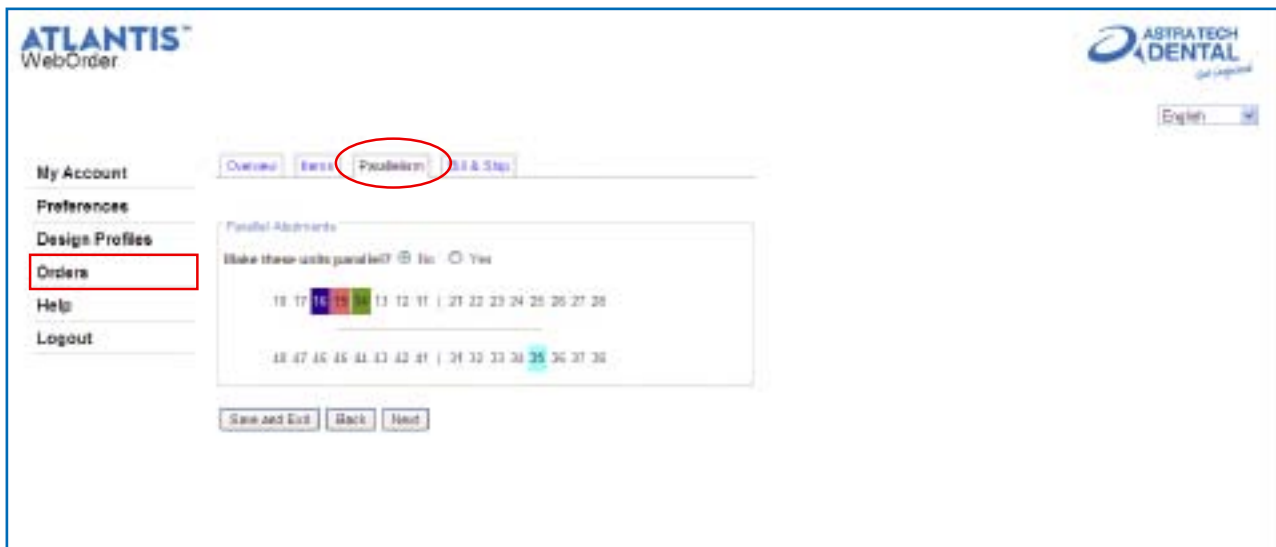

Click **Next** to continue.

Click **Save and Exit** to save your progress and return later to complete your order.

Order page 4 – **Bill & Ship** shows the information previously entered in your preferences.

ATLANTIS™
WebOrder

ASTRA TECH
DENTAL
our support

English

My Account: Overview, Items, Favorites, **Bill & Ship**

Preferences

Design Profiles: **Orders**

Help

Logout

Please review all shipping and billing information for accuracy before submitting your order.

Payment method: Invoice

Shipping preference: Astra Tech selects the best way and of business day.

Bill to:
SEND test
Aggregate 1
Makrid 42121
Sweden
Phone
Fax

Ship to:
Select address from list, or specify new: SEND test

Business name:
Address 1:
Address 2 (optional):
Address 3 (optional):
City:
Postal code:
Country: Sweden
Phone (optional):
Fax (optional):

Back Submit

Click the **Submit** button to complete and send your order electronically to Astra Tech.

Order ticket

Once your Atlantis™ WebOrder is submitted, an **Order ticket** containing a summary of your order information will appear. **Your Order ticket** identifies your case when it is received at Astra Tech.

Print your **Order ticket** by clicking the **Print this** link located at the bottom of the page. Include all items listed under **Case submission check list**.




For easy reference, your Astra Tech customer number will now appear in several areas (including My Account, Order Preferences, under Bill To, and on your order ticket) throughout the Atlantis™ Abutment order process.

Referring to this number when calling in to Astra Tech Customer Service will help us to serve you better.

This **Order ticket** must be signed, packaged with case materials and sent to Astra Tech in order for your case to be processed.

Click **View complete order information** to review all entries for this case.

Click the **Order list** link to return to the **Orders** page where you can check the status of any order entered through Atlantis™ WebOrder.



Hellungatan 1, SE-431 53 Mölndal, Sweden
Telefon +46 31 356 85 00
Email: atlantis_europa@astratech.com

Patient/order ref. 123344
Prescriber:
License:
Phone:

Tooth	Implant type	Abutment Material	Atlantis Gemini™	Parallel Abutments
13	Astra Tech OsseoSpeed 3.5, 4.0 - Aqua	Titanium	<input type="checkbox"/>	P1

Prescribing Clinician or Laboratory Signature: The signature below confirms that this product is being ordered at the request of a licensed dentist or on behalf of a licensed dentist whose information is on file with the laboratory.

Please sign here

Case submission check list
To ensure efficiency in the processing of your order, the following materials are required:

- This Prescription Form
- Articulated Master Casts with analogs placed
- Bite Registration (recommended)
- Model of Soft Tissue

NOTE: Case material(s) must be disinfected prior to shipment.

45444 - SE99001
Bertil Persson
TESTKJND ATL
TEST 123 2
TESTSTADEN, 214 10
Sweden
Phone: 111-111111
Fax:

[Print this](#) | [View complete order information](#) | [Order list](#) | www.astratechdental.com

Hold for design approval

ATLANTIS™
WebOrder



Customer Order #1517491 (HOLD for design approval)

Helander 2211 1 SE 211 53 MINNAPOLIS, Sweden
 Telephone +46 31 386 95 00
 Email order@astratondental.com

Customer Information

Patient or PO Ref: Test case 3E Previous file: AECT ID: 301 Released By: TESTORDD APL UTBILDNING TEST 021 214 9 TEGSTADEN, 214 93 Sweden Phone: 11-111111 Fax: Emailed By: Ed.Larsson_TestEducation@astratond.com	Payment method: Invoice M3-CLING 2305943 Bill To: TESTORDD APL UTBILDNING TEST 021 214 9 TEGSTADEN, 214 93 Sweden Phone: 11-111111 Fax: Ship To: TESTORDD APL UTBILDNING TEST 021 214 9 TEGSTADEN, 214 93 Sweden Phone: 11-111111 Fax: Ship Date: 2019-11-12	Shipped: Shipping preferences: Hold for Tech until the next day and if possible ship #309 69 129 #309 69 129 #309 69 129 #309 69 129 #309 69 129 #309 69 129 #309 69 129
--	---	--

Hold case - send images. (Click on the hold case) additional (if with short design images to get more) [Click on the hold case](#) for more details. [Click on the hold case](#) for more details.

Case Data & Design Preferences

Order Date: 2019-10-01

Item	Implant type	Retention Method	Abutment Geometry	Emergence width	Abutment position	RT	D	BT	L	Chassis	RT In	RT	Parallel Abutments
11	Novo Tech Universal 11 1.1 4.9 Implant	Standard	Standard	Standard	Use Intégral Design	100	0.75	0.75	0.00		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>



Image posted To Oct 06, 2019 at 14:21 (3:22)



Image posted To Oct 06, 2019 at 14:21 (3:23)



Image posted To Oct 06, 2019 at 14:21 (3:22)



Image posted To Oct 06, 2019 at 14:21 (3:23)

Note: Images are available in Atlantis™ WebOrder for 90 days. Images will be expired after 90 days. Please save them on your computer by right clicking over the image and selecting Save as.

Comment on this order

You may enter any notes or comments you have regarding this order in the sample images. Please enter plain text only. HTML is not allowed.

Subject

Is design approval granted?

If **Hold case – send images** was selected during your order entry, you will receive an e-mail notification when your abutment design images are available for your review. Images will be posted to your Atlantis™ WebOrder account.

If you have additional changes, enter your instructions in the comment box and click **Post**. When your revised abutment design images are available, you will receive another e-mail notification.

To indicate your approval for production, click the box next to **Is design approval granted?**

Later orders

Orders for an original Atlantis™ abutment with or without changes to the existing abutment design, or for a separate abutment screw can be placed only after an original order has been shipped. Locate an order by **Case number** from the **Orders** page or search for a **SHIPPED** case. Click the **“Later order”** link under the **Action** column to begin.

Note: A new order number will be generated.

The screenshot shows the Atlantis WebOrder interface. On the left is a navigation menu with 'My Account', 'Orders', 'Help', and 'Logout'. The main area features 'Atlantis™ 3D Editor' with a 'New available!' callout. Below this is an 'Advanced Search' section with a dropdown menu set to 'SHIPPED' and a 'Search' button. A table of orders is displayed below, with the 'Action' column containing 'Later order' links for each row. Two of these links are circled in red.

Patient/order ref.	Prescriber	Units	Submit date	Materials received	Due date	Status	Case number	Atlanta™ abutment core file	Action
AWO 5.18.0 (1/0)	Petra	1	2011-10-20	2011-10-26	2011-11-02	SHIPPED	1554018		Later order
AWO original 2		2	2011-08-18			SHIPPED	1554401		Later order
AWO original 1		3	2011-08-18			SHIPPED	1554366		Later order
AWO later test 1		1	2011-08-14	2011-08-14	2011-08-30	SHIPPED	1554382		Later order
AWO patient name		1	2011-01-17			SHIPPED	1525891		Later order
AWO patient name (2 new comments)		1	2011-01-08	2011-01-08	2011-01-10	SHIPPED	1425068		Later order
AWO patient name	Petra	1	2010-08-02	2010-08-05	2010-08-10	SHIPPED	1525721		Later order

You will have three choices on the **Later order** page:

The screenshot shows the 'Later order' page in the Atlantis WebOrder interface. It prompts the user to 'Select one of the options below:' and provides three choices:


- Screws**
 - [Abutment screw](#)
 - Order a separate screw for any of the original abutment(s) ordered
 - Shipping information editable
- Abutments**
 - [No rescan required](#)
 - Duplicate - no changes to the original abutment(s) ordered
 - Change in material type and/or minimal design changes
 - Shipping information editable
 - [Rescan required](#)
 - Significant design changes
 - New case material must be sent in
 - All selections and preferences are editable

Abutment screw

You can order a separate abutment screw without ordering an abutment.

Click on the **Abutment screw** link to open the **Overview** page. Confirm the **Patient** and **Prescriber** information and select the appropriate tooth or teeth for which you would like to order a separate abutment screw. **Note!** Uncheck if you don't want screws for all implants.


Confirm the order by clicking the **Submit** button or click **Next** to modify the **Bill & Ship** information.

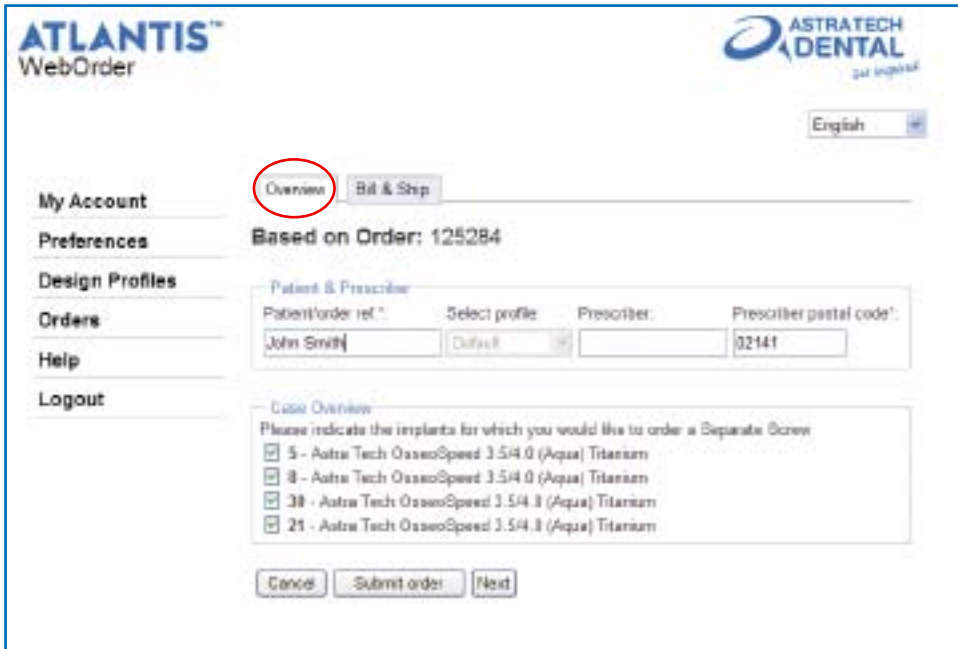

No rescan required

For later orders with no/minimal design changes to the original abutment(s) ordered, and/or change in material type, click on **No rescan required**.

Order page 1 – Overview will display the original case number and all data from the original case. Data can be changed except for those in grayed out fields.

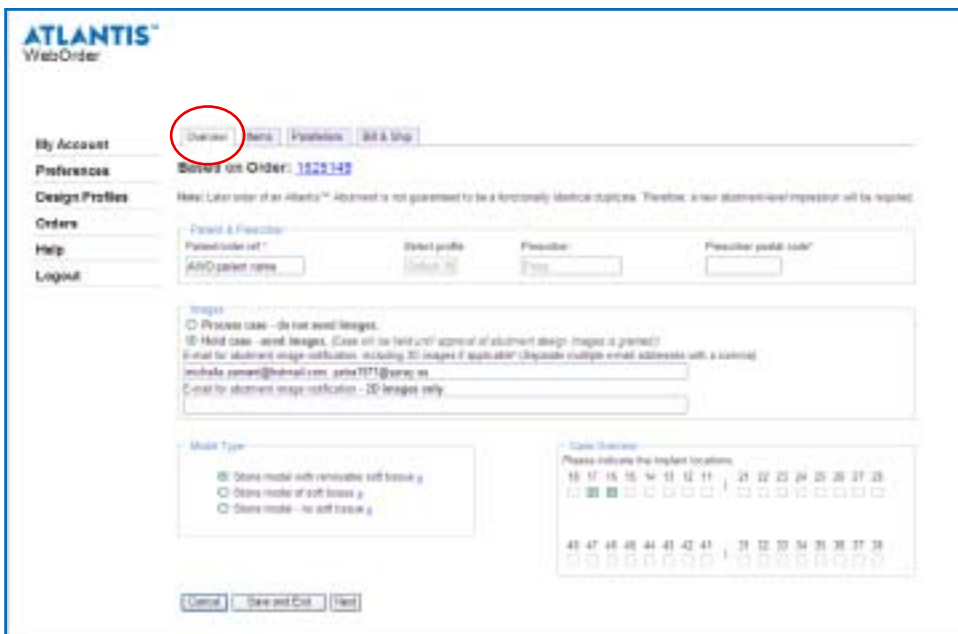


Order page 2 – Items will display all data from the original case.

All preferences are editable except implant type as this would require a rescan of the case.

Note: If you need to revert to the original order data, click the **Reset values to original settings** link.

You can add new notes in the **Additional Case Instructions** field provided. Previous case notes will be available as read-only in the **Previous Case Instructions** field for your reference.

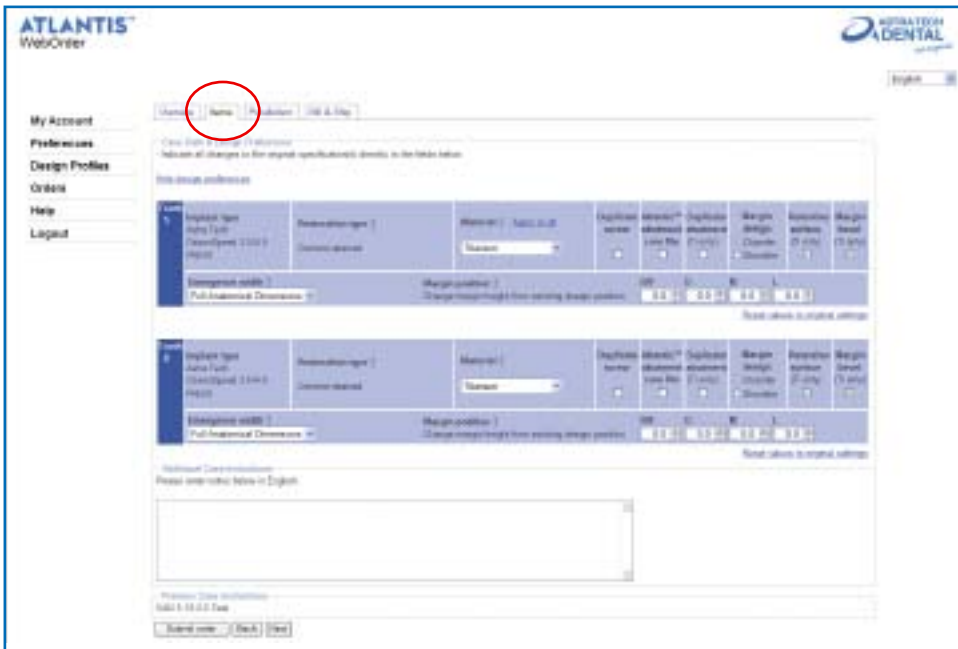


Order page 3 – Parallelism

If some, but not all, units are selected from a parallel group, the page will be displayed, but no changes will be allowed. If all the units from a parallel group are selected, the page will be displayed and changes will be allowed.



Later orders


Order page 4 – Bill & Ship shows the remaining information populated from your original order. To ensure accuracy, review all information in detail before submitting your order. All fields are editable.

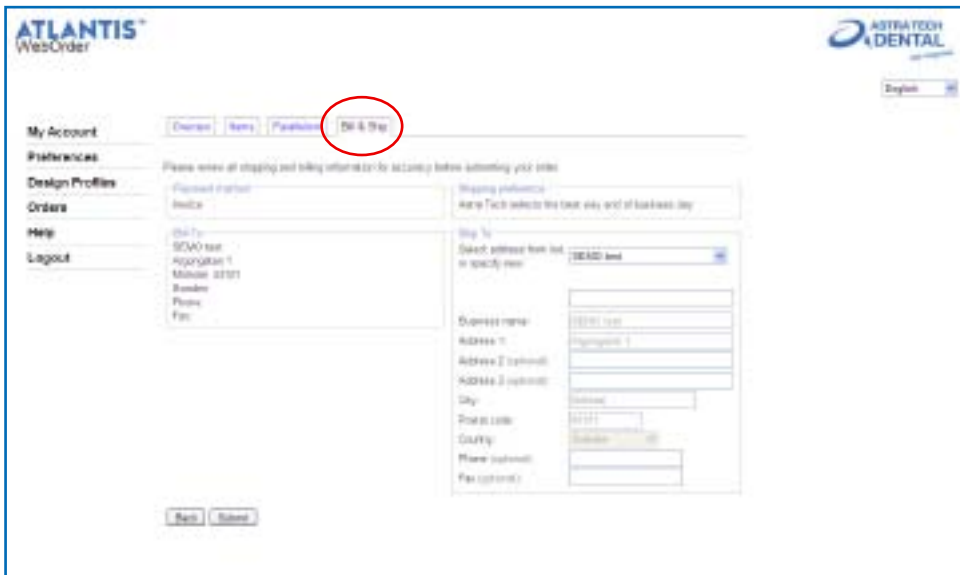

Rescan required

For later orders with significant design changes to the original abutment(s) or changes such as implant type, new case material must be sent in. Click on **Rescan required**.


Order page 1 – Overview will display the original case number and all data from the original case. Data can be changed except for those in grayed out fields.

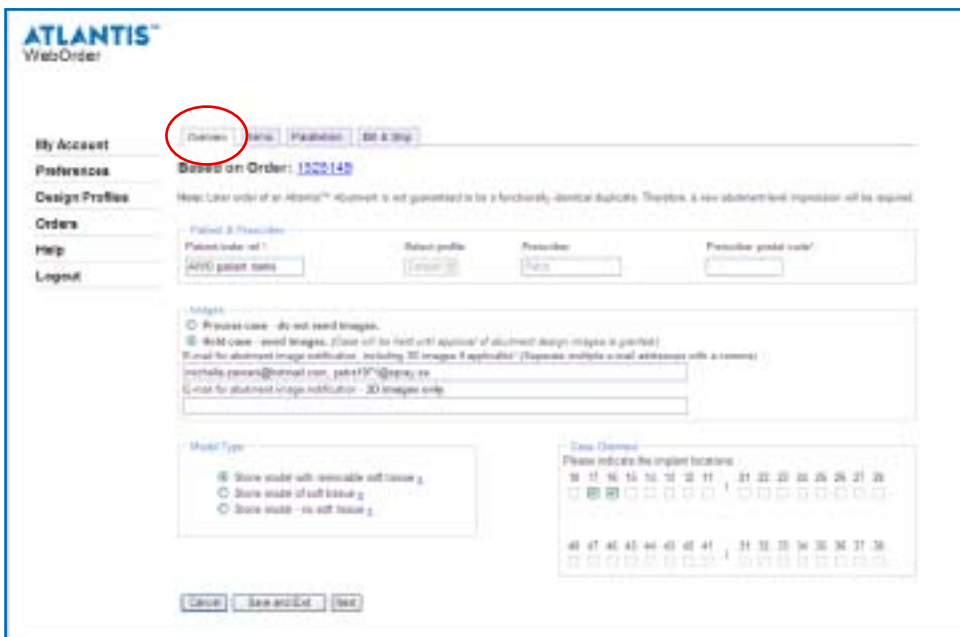

Order page 2 – Items will display all data from the original case, all of which can be edited.

Note: If you need to revert to the original order data, click the **Reset values to original settings** link.

You can add new notes in the **Additional Case Instructions** field provided. Previous case notes will be available as read-only in the **Previous Case Instructions** field for your reference.

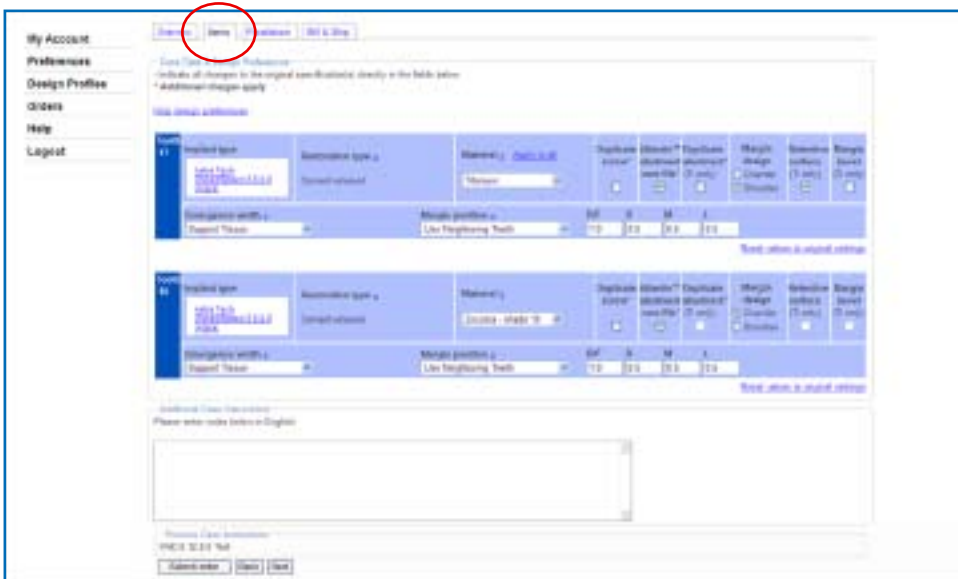

Order page 3 – Parallelism

If some, but not all, units are selected from a parallel group, the page will be displayed, but no changes will be allowed. If all the units from a parallel group are selected, the page will be displayed and changes will be allowed.



My account

On the **My Account** page, the account manager can edit account information by clicking the **Edit this information >>** link and add new users by clicking the **Add new user >>** link.

ATLANTIS™ WebOrder

ASTRATECH DENTAL

English

My Account My Account

Preferences

Design Profiles

Orders

Help

Logout

Name - Tony Test
 Email - tonytest1@astratech.com
 Time format - 11:59 PM (EST)
 Time zone - (GMT-05:00) Eastern Time (US & Canada)
 Send email notification for images - All orders entered
 Atlantis™ 3D Viewer - Enabled

[Edit this information >>](#)

Ordering Address (To change this information, contact Astra Tech Customer Service at +46 31 336 05 00)

Edit account information as needed and then click the **Save** button to return to the **My Account** page.

Use **Send email notification for images** to indicate whether the user should receive an email notification for either:

- None: No cases – not even the ones that the User enters
- Orders entered by this user only – images for just the cases that the User has entered
- All orders entered – regardless of which User entered the case.

Atlantis™ 3D Viewer can be enabled or disabled for all Users of an Account by the Account Manager only. **Note:** If the Atlantis 3D Viewer option is enabled for the account, each User can set their personal preference to either keep the feature enabled or to disable it. This allows for more convenience and customization per work station.

ATLANTIS™ WebOrder

ASTRATECH DENTAL

English

My Account Edit My Account

Preferences

Design Profiles

Orders

Help

Logout

User

First name: Education
 Last name: Test
 Email: education1@astratech.com

Preferences

Time format: 11:59 PM (CET)
 Time zone: (GMT+01:00) CEST

Send email notification for images

None
 Orders entered by this user only
 All orders entered

Atlantis™ 3D Viewer

Enabled
 Disabled

Save

[Change password >>](#)

If you have questions, please contact Astra Tech Customer Service at +46 31 336 05 00

Edit account information as needed and then click the **Save** button to return to the **My Account** page.

ATLANTIS™ WebOrder

ASTRATECH DENTAL
get inspired

English

My Account Edit My Account

Preferences

Design Profiles

Orders

Help

Logout

User

First name: Education

Last name: Test

Email: education1@astratech.com

Time format: 11:59 PM (CET)

Time zone: (GMT+01:00) Bonn

Send email notification for images:

None

Orders ordered by this user only

All orders ordered

Atlantis™ 3D Viewer

Enabled

Disabled

Save

[Change password >>](#)

If you have questions, please contact Astra Tech Customer Service at +46 31 350 95 08

To change your password, click the **Change password >>** on bottom of the **My Account** page.

Fac: tomybert1@tobmail.com

ACCOUNT USERS

User	Email	Status	Delete
to mybert1@tobmail.com	to mybert1@tobmail.com	Act. Mgr	

[Add new user >>](#)

You as Account Manager may:

To add a new user, enter the first name, last name and email address of the user. Click **Register** to add the new user. You will be redirected back to **My Account** page.

The new user will receive an email to confirm their account.

Each user can access the same account but with different passwords, providing added flexibility in working with Atlantis™ WebOrder.

ATLANTIS™ WebOrder

ASTRATECH DENTAL
get inspired

English

My Account

Preferences

Design Profiles

Orders

Help

Logout

New user for EU Dental account

User

First name: []

Last name: []

Email: []

Language: English

Register

Preferences

Order preferences may be changed by clicking on the **Edit this information** link on the **Order Preferences** page.

ATLANTIS™ WebOrder **ASTRATECH DENTAL**
get inspired

My Account English

Preferences

SEMO test ACCOUNT

Order Preferences

- Images - Select per case (No users designated to receive image notification)
- Adjustment material - None
- Atlantis™ 3D Views - Enabled
- Shipping carrier - Astra Tech selects the best way
- Shipping preference - end of business day
- Payment method - Invoice

Saved Billing Addresses

Business name	Address	Numbers	Default
SEMO test	Aggatan 1 + Möadal 42121 Sweden	Phone: Fax:	

Saved Shipping Addresses

Business name	Address	Numbers	Default
SEMO test	Aggatan 1 + Möadal 42121 Sweden	Phone: Fax:	

[Edit this information](#)

ATLANTIS™ WebOrder **ASTRATECH DENTAL**
get inspired

My Account English

Preferences

Edit Preferences

Images

- Process case - do not send images
- HMI case - send images
- Select per case

Atlantis™ 3D Views

- Enabled
- Disabled

Shipping carrier

Astra Tech selects the best way

Payment method

Invoice

Adjustment material

- Titanium
- Gold-plated titanium
- Zirconia - white
- Zirconia - shaded
- Select per case

Shipping preference

Astra Tech selects the best way end of business day

Billing addresses

SEALITE
TESTFUND ATL UTBIUMING
TEST 123 2
214 10 TESTSTADEN 214 10
Sweden
Phone: 111-111111
Fax:

Shipping addresses

TESTFUND ATL UTBIUMING

SEALITE
TEST 123 2
214 10 TESTSTADEN 214 10
Sweden
Phone: 111-111111
Fax:

Save

Once edited, click **Save** to return to **Order Preferences**.

Design profiles

On the **Design Profiles** page you may **add preferences**, **Enter a new profile >>** or **delete profile**.

ATLANTIS™ WebOrder

ASTRATTECH DENTAL
our support

English

My Account

Preferences

Design Profiles

Orders

Help

Logout

Design Profiles

[Create new profile >>](#)

Profile name: Default

Create for instance

[Add a new!](#)

Dental Region	Emergence width	Margin position	B.F.	D.	M.	L.	Margin Design	Retentive surface	Margin Bevel	Delete?
Default	Contour Soft Tissue Use Subgingival Depth	1.8	8.75	0.75	0.8		Chamber	True	False	
Max. Anatomic	Contour Soft Tissue Use Subgingival Depth	1.8	8.75	0.75	0.8		Chamber	True	False	x
Max. Anatomic	Contour Soft Tissue Use Subgingival Depth	1.8	8.75	0.75	0.8		Chamber	True	False	x
Max. Prosthetic	Contour Soft Tissue Use Subgingival Depth	1.8	8.75	0.75	0.8		Chamber	True	False	x

[add preference](#)

Profile name: AT Dent

Create for instance

Show [0/1/2] [Add a new!](#) [Cancel](#)

Dental Region	Emergence width	Margin position	B.F.	D.	M.	L.	Margin Design	Retentive surface	Margin Bevel	Delete?
Default	Contour Soft Tissue Use Subgingival Depth	1.8	8.75	0.75	0.8		Chamber	True	False	
add preference										

[delete profile](#)

Add preferences

On the **New Design Preference** page, you may edit and save your default for preferences such as **Emergence Width Options** and **Margin Position Options**. All defaults can also be modified on an order-by-order basis as needed.

When new defaults have been set, click **Create**.

The screenshot shows the 'New Design Preference' page in the ATLANTIS WebOrder system. The 'Design Profiles' menu item is highlighted in red. The 'Emergence Width Options' section is circled in red, showing radio buttons for 'Full Anatomical Dimensions', 'Contour Soft Tissue', 'Support Tissue', and 'No Tissue Displacement'. The 'Margin Position Options' section is also circled in red, showing radio buttons for 'Use Sulcus/Depth', 'Use Height/ing Teeth', 'Use Heights Above Interface', and 'As Close to Interface as Possible'. The 'Physical Features' section includes checkboxes for 'Margin design', 'Shoulder', 'Chamfer', 'Retentive Surface for Titanium', and 'Margin bevel'. A 'Create' button is circled in red at the bottom left.

Emergence width options

Full anatomical dimensions

Largest diameter abutment provided with the best emergence profile possible. A surgical incision for placement may be required.

Contour soft tissue

Medium diameter anatomically shaped abutment up to 1.0 mm larger than sulcus of model of the soft tissue model provided.

Support tissue

Anatomically shaped abutment that may be up to 0.2 mm larger than sulcus of the soft tissue model provided with desired emergence profile. "Easy" insertion.

No tissue displacement

Smallest diameter, non-anatomically shaped abutment with no soft tissue support. The abutment will not touch the soft tissue.

Enter a new profile

A new design profile can be created using a customer name or other identifier. Selecting a specific design profile on the Overview page automatically uses the preferences specified for that profile. Click the link for **Enter new profile**, type in the profile name and click **Create**.

ATLANTIS™ WebOrder

ASTRATECH DENTAL

English

My Account

Preferences

Design Profiles

Orders

Help

Logout

New Design Profile

Design profile for prescriber:

Email address (optional):

Phone ZIP (optional):

Create

After creating a new profile you may customize the profile by selecting the **Add preference** link under the Profile to access the **New Design Preference** page. (See previous page for details.)

ATLANTIS™ WebOrder

ASTRATECH DENTAL

English

My Account

Preferences

Design Profiles

Orders

Help

Logout

New Design Preference

Dental region for preference: Max. Anterior

Emergency Width Options

Full Anatomical Dimensions

Contour Soft Tissue

Support Tissue

No Tissue Displacement

Margin Position Options

Use Subgingival Depth

BF	D	M	L
1.0	0.75	0.75	0.5

Use Neighboring Teeth

Use Heights Above Interface

BF	D	M	L
1.0	1.5	1.5	1.0

As Close to Interface as Possible

Physical Features

Margin design

Shoulder

Chamfer


Retentive Surface for Titanium

Margin bevel


Create

Help overview

Visit the **Help** section at any time during the ordering process for additional information related to ordering an Atlantis™ abutment, such as shipping instructions, articulator guide and turnaround time calculator.

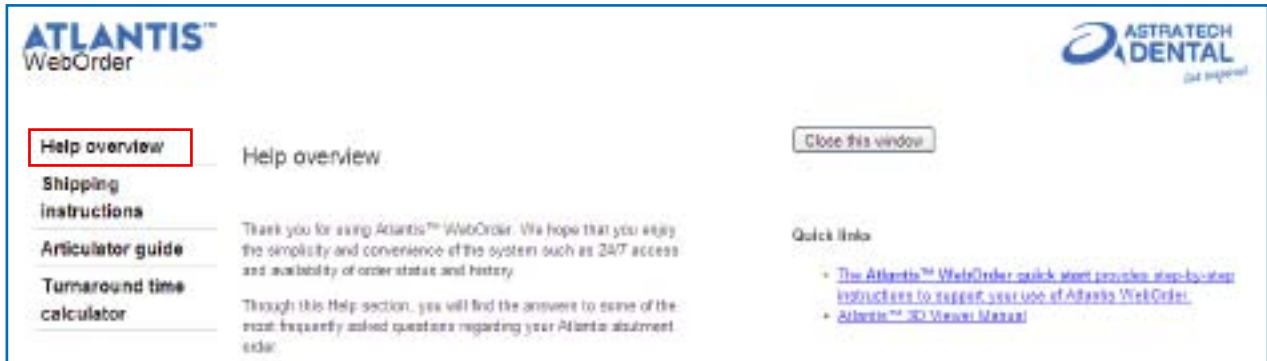

Clicking on any of the **>>** within Atlantis™ WebOrder brings up a graphic illustration of the option.

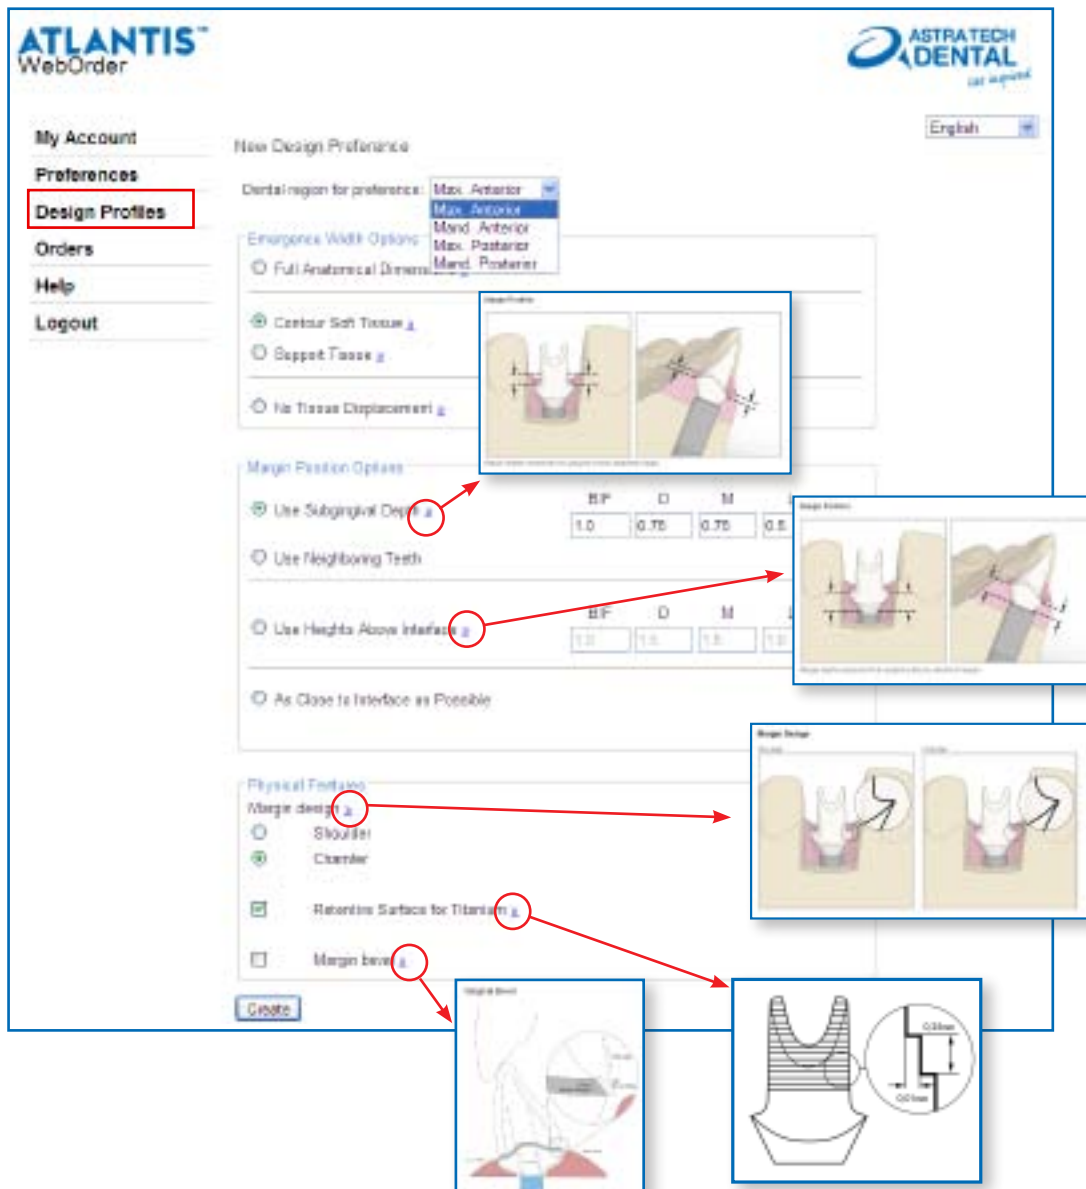

Emergency Width Options

The screenshot shows the 'New Design Preference' page for 'Emergency Width Options'. The options are:

- Full Anatomical Dimensions
- Contact Soft Tissue
- Support Tissue
- No Tissue Displacement

Each option has a right-pointing arrow icon. Red arrows point from these icons to corresponding graphic illustrations on the right side of the page. The illustrations show cross-sections of dental abutments with different tissue levels and widths.

Clicking on any of the **>>>** brings up an graphic illustration of the option.
See "Design guide – Atlantis™ patient-specific abutments" manual for more information.

Model Type

The screenshot shows the 'Model Type' section of the Atlantis WebOrder. The options are:


- Store model with overbite
- Store model of soft tissue
- Store model - no soft tissue

Below the options is a 'Tooth Positions' grid. Red arrows point from the radio buttons to corresponding photographs of dental models on the right. The first photo shows a model with a pink wax overbite. The second photo shows a model with a metal abutment and a circular callout indicating a 0.3mm gap. The third photo shows a model with a metal abutment and a circular callout indicating a 0.3mm gap.

Atlantis BioDesign Matrix™

Atlantis™ is comprised of a unique combination of four key features, known as the Atlantis BioDesign Matrix™. These features work together to support soft tissue management for ideal functional and esthetic result. This is the true value of Atlantis™ for dental laboratories, clinicians and implant patients.

- **Atlantis VAD™** – designed from the final tooth shape and the individual patient anatomy.
- **Natural Shape™** – shape and emergence profile based on individual patient anatomy.
- **Soft-tissue Adapt™** – optimal support for soft tissue sculpturing and adaptation to the finished crown.
- **Custom Connect™** – strong and stable fit – customized connection for all major implant systems.

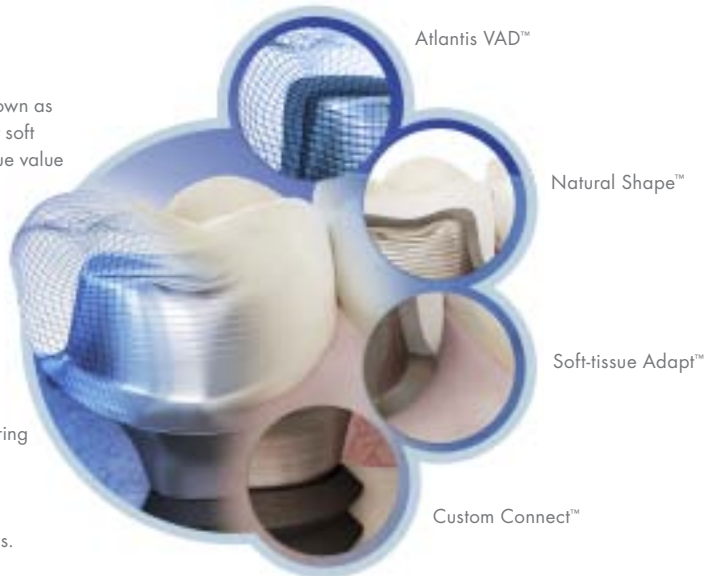

Australia

Astra Tech Pty Ltd.
Suite 1, 53 Grandview St, Pymble NSW 2073
☎ +61 2 9488 3500. 📠 +61 2 9440 0744
www.astratechdental.com.au

Austria

Astra Tech GesmbH
Schloßhofer Straße 4/4/19, AT-1210 Wien
☎ +43-(0)1-2146150. 📠 +43-(0)1-2146167
www.astratechdental.at

Benelux

Astra Tech Benelux B.V.
Signaalrood 55, NL-2718 SG Zoetermeer
☎ +31 79 360 1955/+32 3 232 81 50
📠 +31 79 362 3748/ +32 3 213 30 66
www.astratechdental.nl

Canada

Astra Tech Inc.
2425 Matheson Blvd East, 8th Floor
Mississauga, ON L4W 5K4
☎ +1 905 361 2844
www.astratechdental.com

Denmark

Astra Tech A/S
Roskildevej 163, 1. th., DK-2620 Albertslund
☎ +45 43 71 33 77. 📠 +45 43 71 78 65
www.astratechdental.dk

East Asia

Astra Tech
Suite 15.02, 15th Floor Menara PanGlobal
No. 8 Lorong P Ramlee, MY-50250, Kuala Lumpur
Malaysia
☎ +60 3 27 11 2531. 📠 +60 3 27 11 2532
www.astratechdental.com

Finland

Astra Tech Oy
PL 96, FI-02231 Espoo
☎ +358 9 8676 1626. 📠 +358 9 804 4128
www.astratechdental.fi

France

Astra Tech France
7, rue Eugène et Armand Peugeot, TSA 90002
FR-92563 Rueil Malmaison Cedex
☎ +33 1 41 39 02 40. 📠 +33 1 41 39 02 44
www.astratechdental.fr

Germany

Astra Tech GmbH
An der kleinen Seite 8. DE-65604 Elz
☎ +49 6431 9869 0. 📠 +49 6431 9869 500
www.astratechdental.de

Italy

Astra Tech S.p.A.
Via Cristoni, 86, IT-40033 Casalecchio di Reno (BO)
☎ +39 051 29 87 511. 📠 +39 051 29 87 580
www.astratechdental.it

Japan

Astra Tech K.K.
Yaesuguchi-Daiei Building 12F
1-3-1 Kyobashi, Chuo-ku, Tokyo 104-0031
☎ +81 3 3243 5055. 📠 +81 3 3243 5057
www.astratech.jp

Norway

Astra Tech AS
Karihaugveien 89, NO-1086 Oslo
☎ +47 67 92 05 50. 📠 +47 67 92 05 60
www.astratechdental.no

Poland

Astra Tech Sp.z o.o.
ul. Orężna 58, PL-02-937 Warszawa
☎ +48 22 853 67 06. 📠 +48 22 853 67 10
www.astratechdental.pl

Portugal

Astra Tech
Lagoas Park, Edifício 8 – 1º piso
PT-2740-268 Porto Salvo
☎ +351 21 421 2273. 📠 +351 21 421 0234
www.astratechdental.pt

Spain

Astra Tech S.A.
Calle Ciencias nº 73 derecha. Nave 9,
Poligono Industrial Pedrosa,
ES-08908 L'Hospitalet de Llobregat
☎ Servicio al cliente: +34.902.101.558
☎ +34.932.643.560. 📠 +34.933.363.231
www.astratechdental.es

Sweden

Astra Tech AB
P.O. Box 14, SE-431 21 Mölndal
☎ +46 31 776 30 00. 📠 +46 31 776 30 17
www.astratechdental.se

Switzerland

Astra Tech SA
Avenue de Sévelin 18, P.O. Box 54
CH-1000 Lausanne 20
☎ +41 21 620 02 30. 📠 +41 21 620 02 31
www.astratechdental.ch

United Kingdom

Astra Tech Ltd.
Brunel Way, Stonehouse, Glos GL10 3SX
☎ +44 845 450 0586. 📠 +44 1453 791001
www.astratechdental.co.uk

USA

Astra Tech Inc.
590 Lincoln Street, Waltham, MA 02451
☎ +1-800-531-3481. 📠 +1-781-890-6808
www.astratechdental.com

Other Markets

Astra Tech AB, Export Department
P.O. Box 14, SE-431 21 Mölndal, Sweden
☎ +46 31 776 30 00. 📠 +46 31 776 30 23
www.astratechdental.com



Astra Tech AB, Aminogatan 1, P.O. Box 14, SE-431 21 Mölndal, Sweden
☎ +46 31 776 30 00. 📠 +46 31 776 30 10. www.astratechdental.com